


Prove di laboratorio

TOTAL BODY con TecnoScan




ABBATTIMENTO Ampiezza/Frequenza

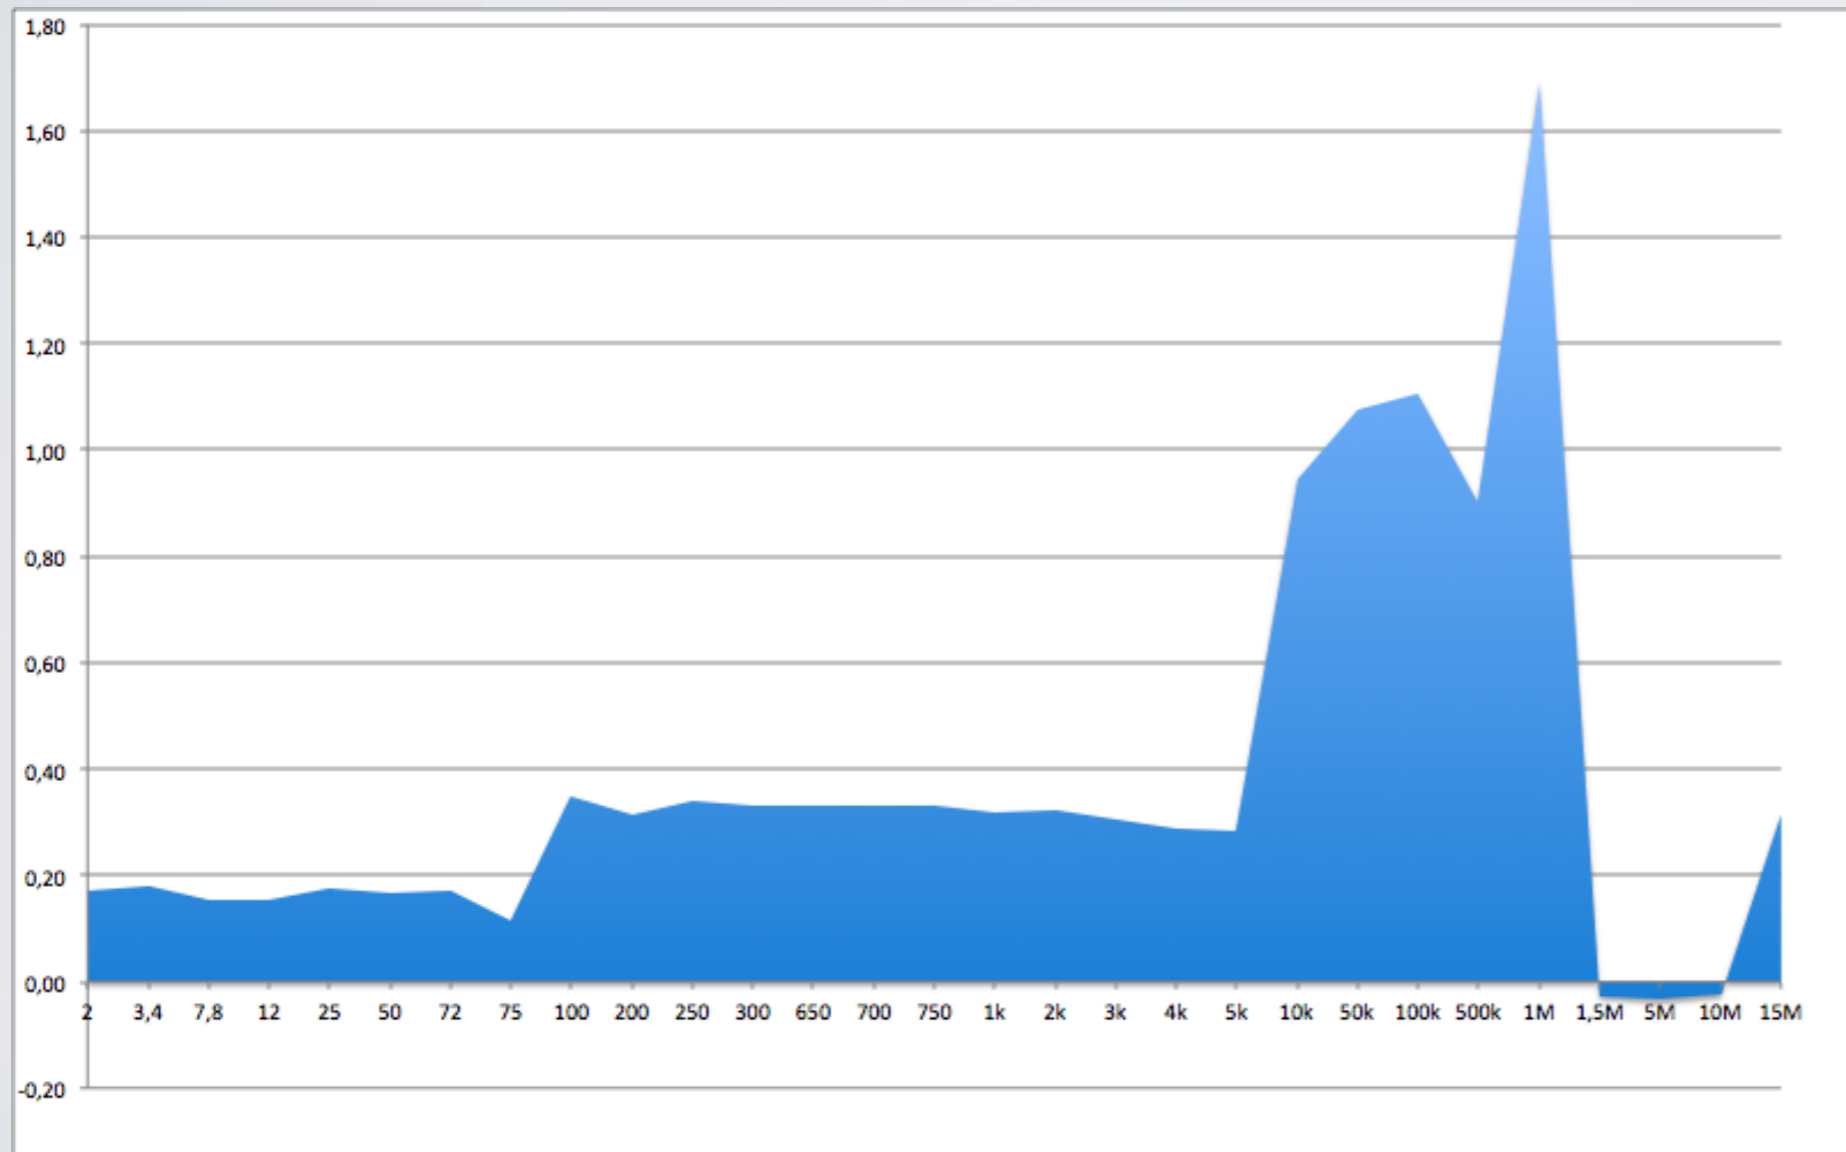

FREQUENZA	%
2	1,99
3,4	2,95
7,8	1,00
12	1,18
25	3,00
50	2,32
72	2,75
75	0,98
100	23,88
200	21,86
250	23,33
300	22,88
650	22,96
700	22,78
750	22,95
1k	22,68
2k	22,69
3k	21,51
4k	20,47
5k	20,16
10k	47,77
50k	51,03
100k	51,68
500k	46,48
1M	61,68
1,5M	-3,53
5M	-3,86
10M	-3,61
15M	21,67

HF: alta frequenza



SPETTRO

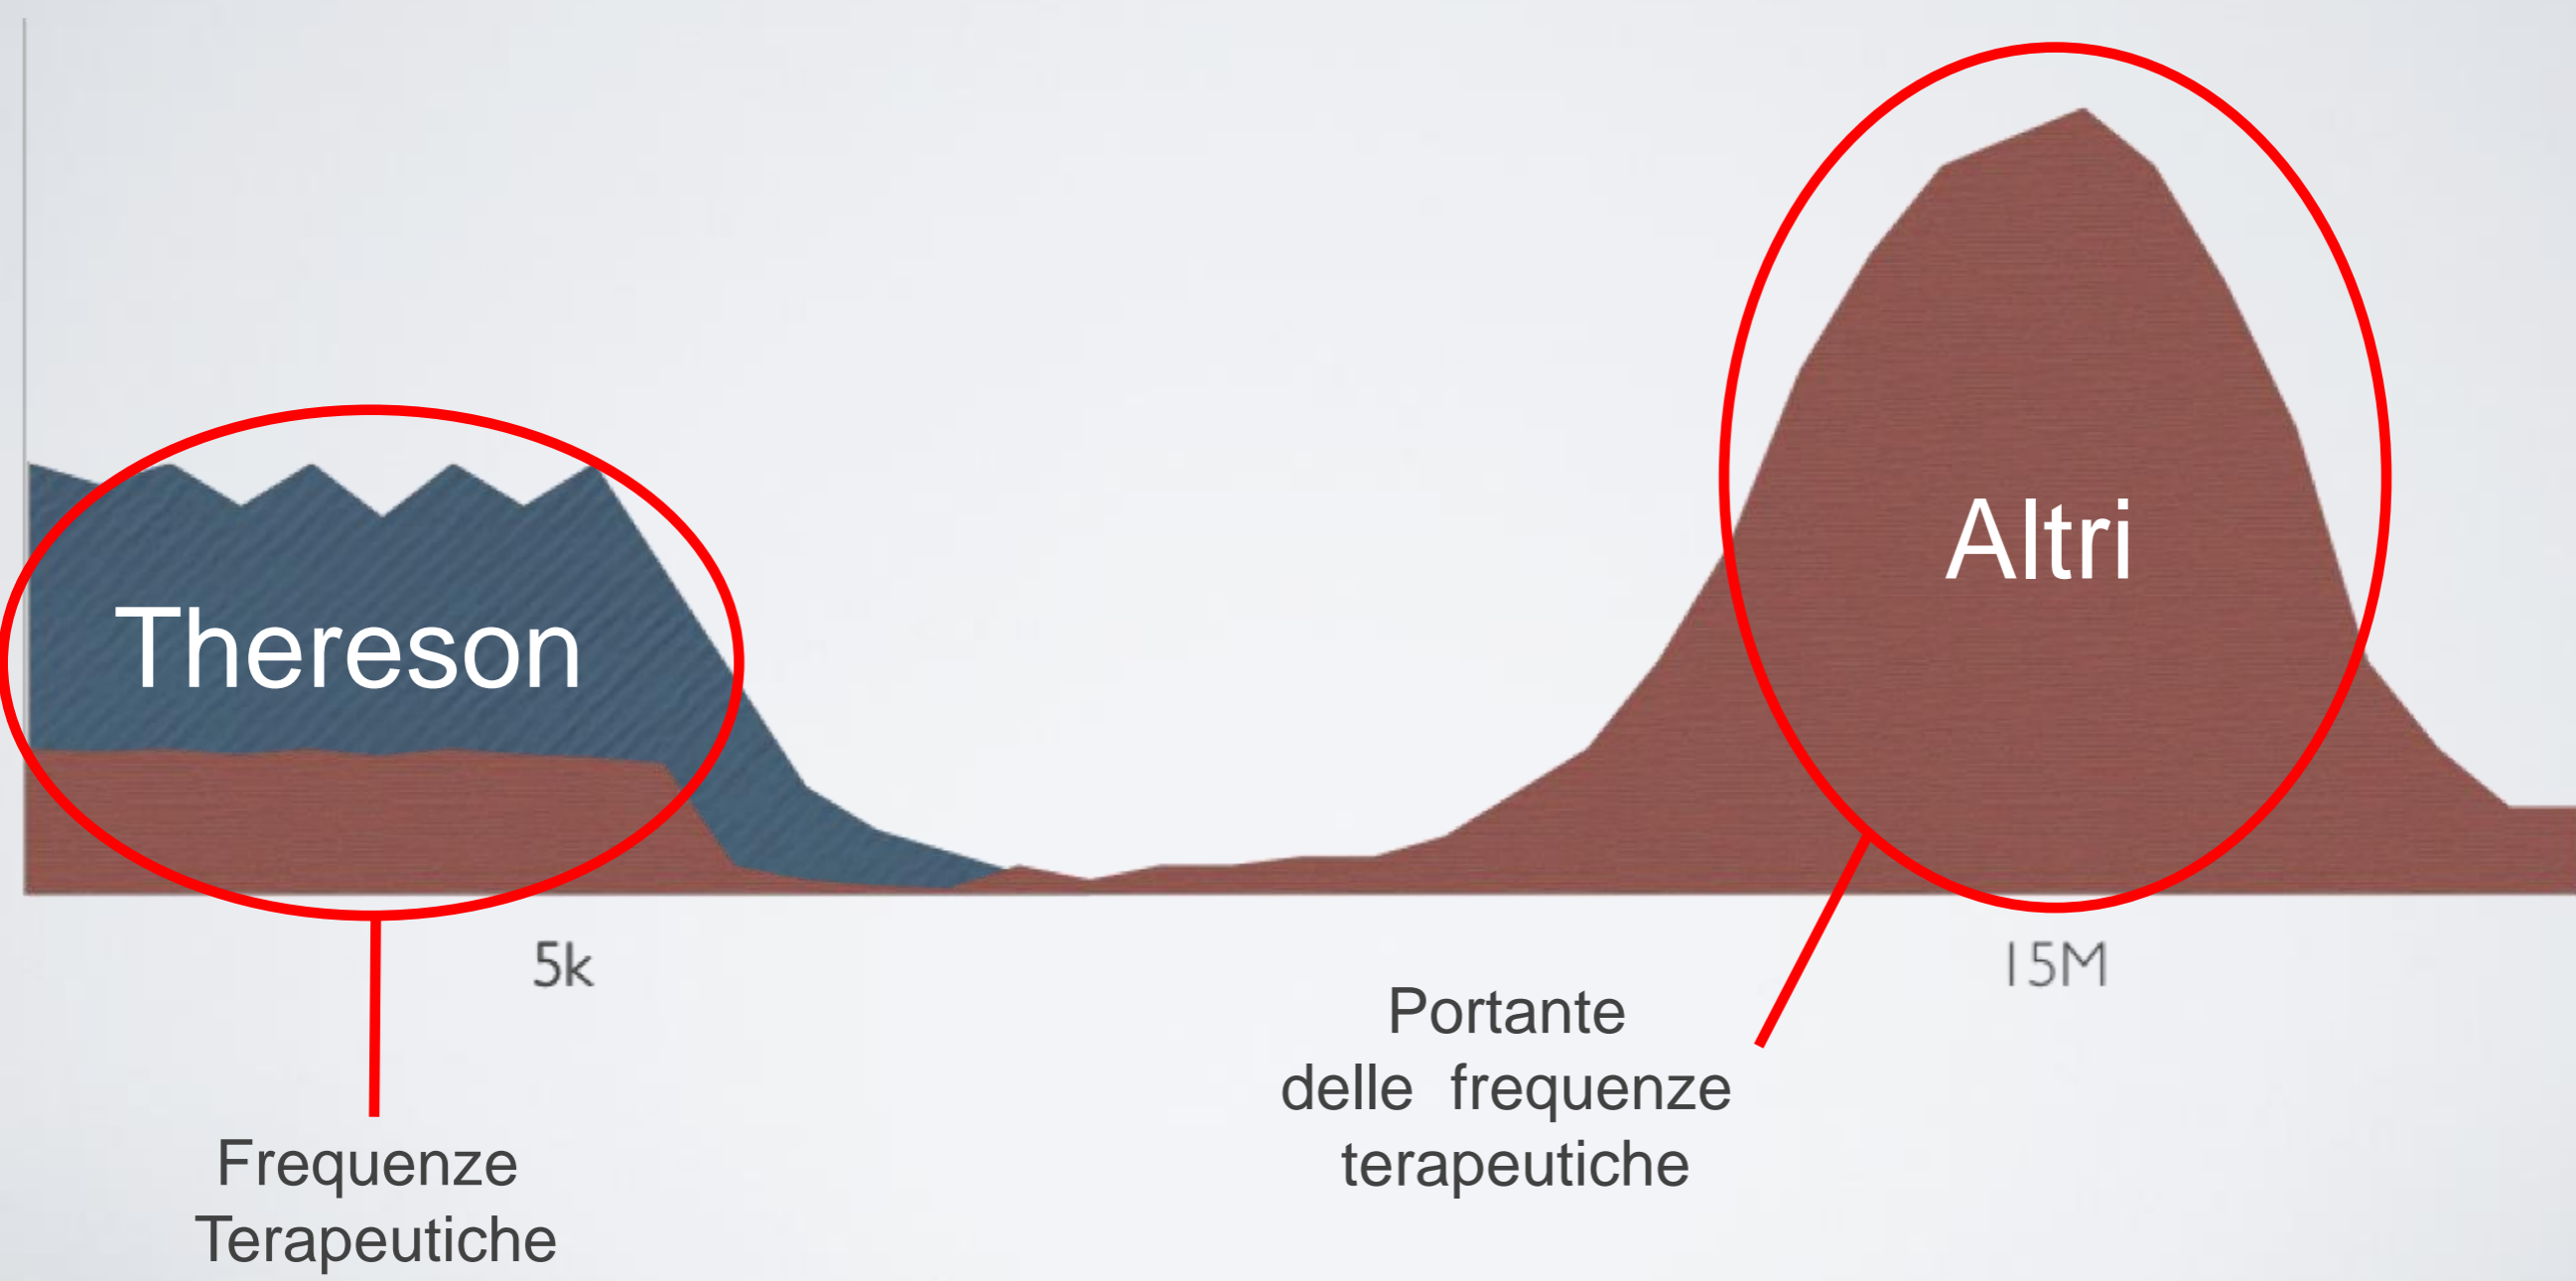

TOTAL BODY

THERESON
THERAPEUTIC MAGNETIC RESONANCE

Efficace nelle alte frequenze

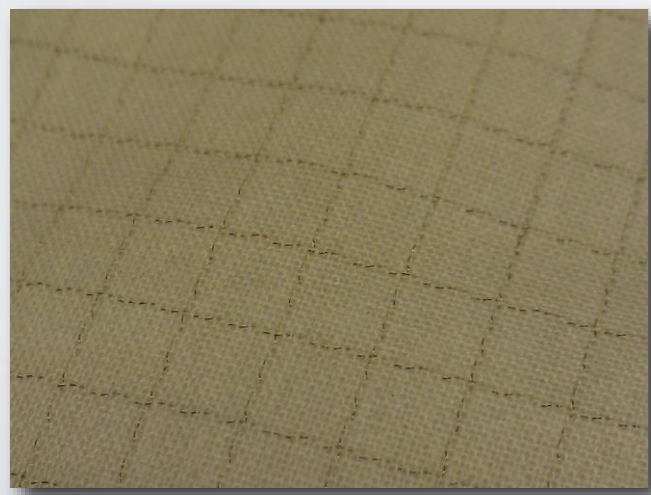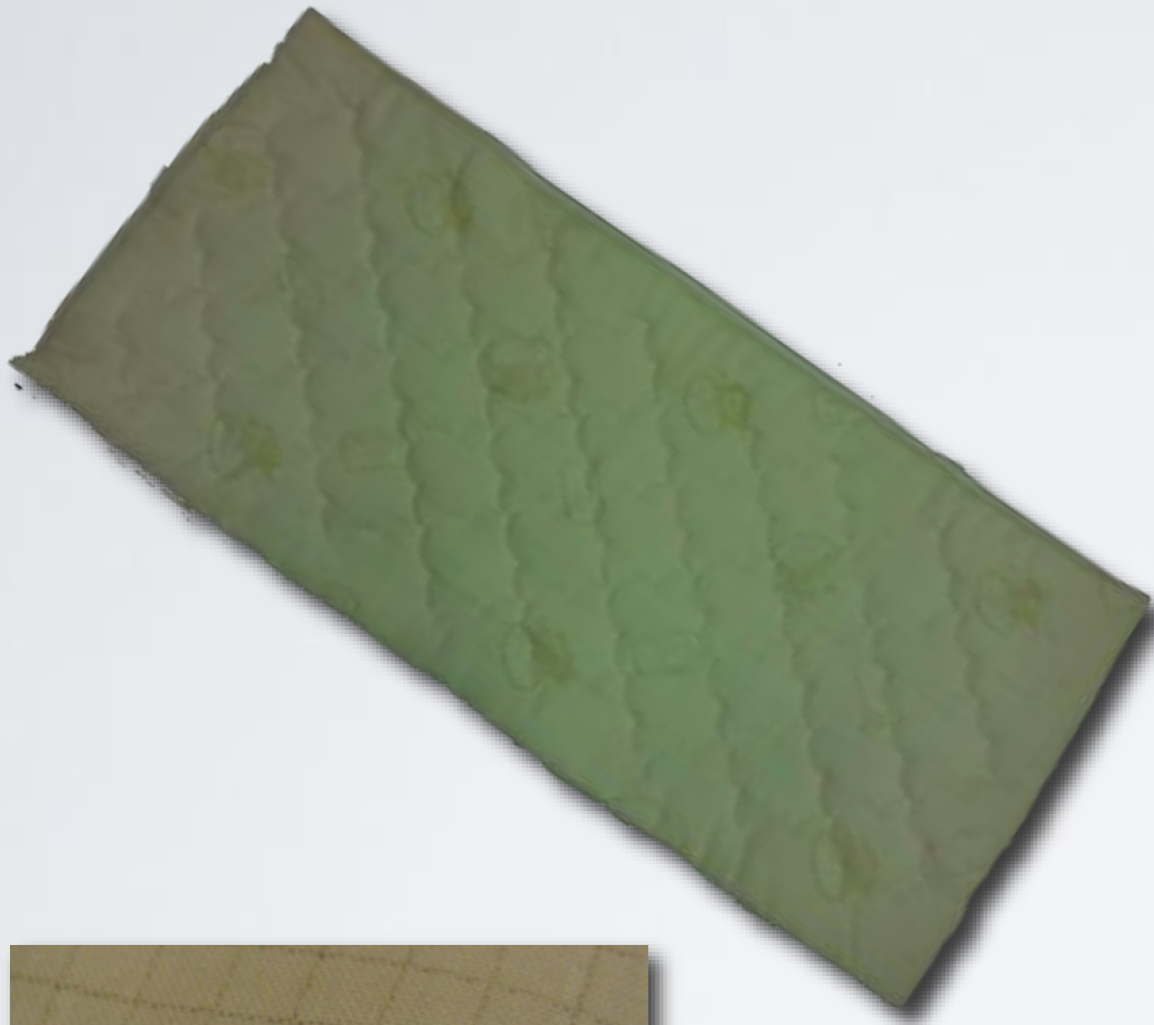

- Efficace alle alte frequenze
- L' unico con magnetoterapia
- Abbattimento smog EM
- 6 solenoidi (rame indeform.)
- Generazione di campo totale

THERESON

THERAPEUTIC MAGNETIC RESONANCE

R & D

Grazie